
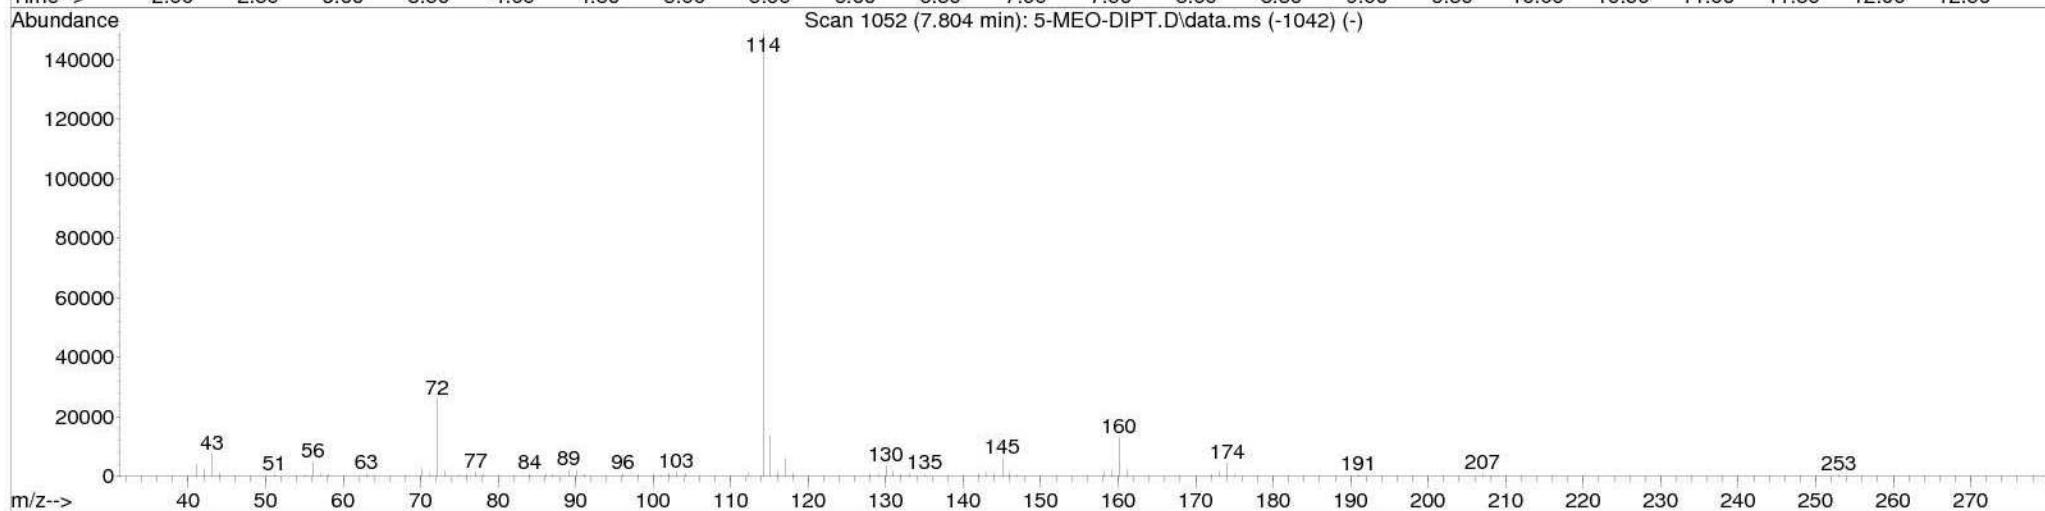


Name of File: D:\Data\JABPDF\00Edited\5-MEO-DIPT.D  
Method: 90\_1\_30.M  
Misc Info: DEA# 361601 30m HP-5 MS, 0.25mm / DEA SWL

Vial Number: 57  
Instrument: DEA# 361782

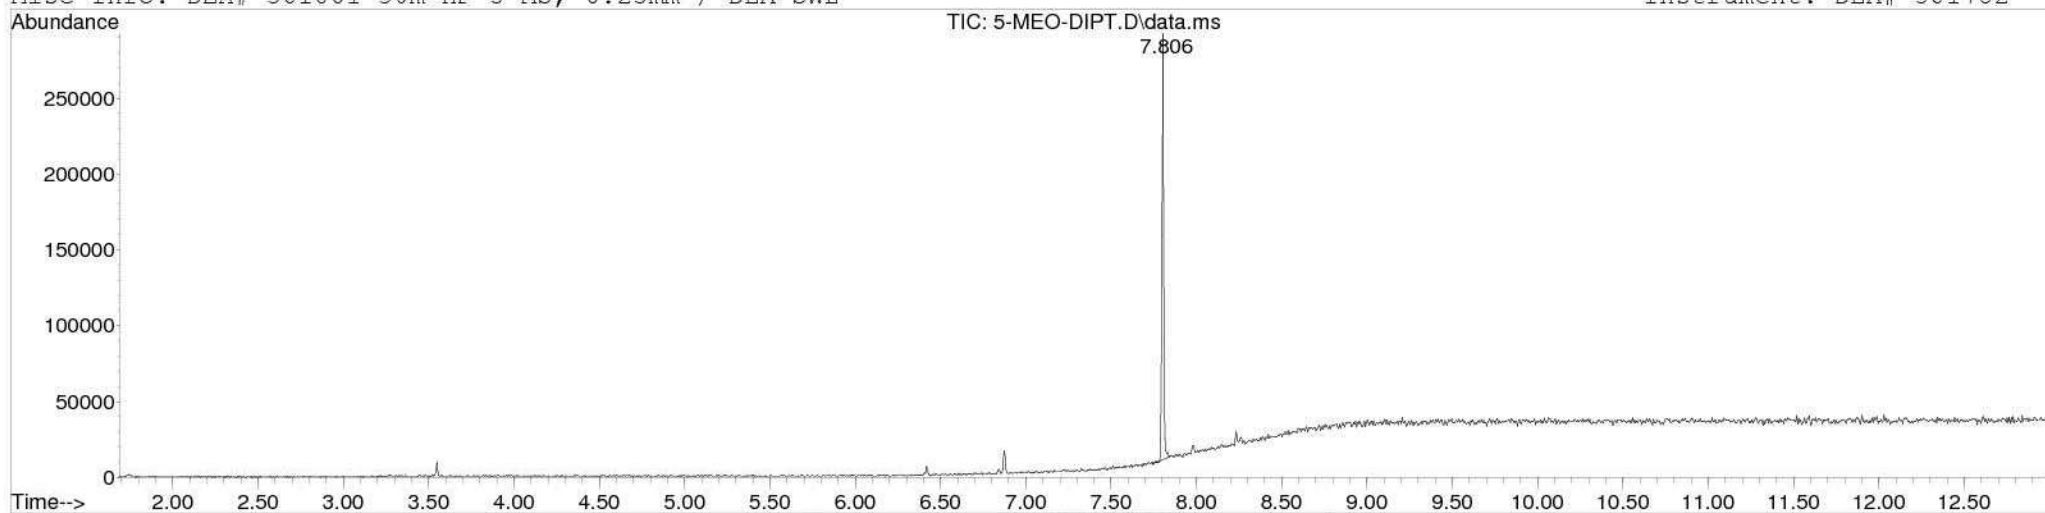

INSTRUMENT CONDITIONS

temp: 90 °C for 1.0 min  
then 30 °C/min to 300 °C for 5.0min

Run Time 13.0 min  
inj. port: 280 °C, transfer line: 280 °C  
GC column: HP-5MS: 30 m x 250 µm x 0.25 µm film  
split mode: Split, ratio: 50 :1  
tune: stune.u , multiplier offset: 0V

MS ACQUISITION PARAMETERS film

Laboratory Number: 5-MeO-DIPT  
Date: 25 May 2004 14:03  
Initials: \_\_\_\_\_