
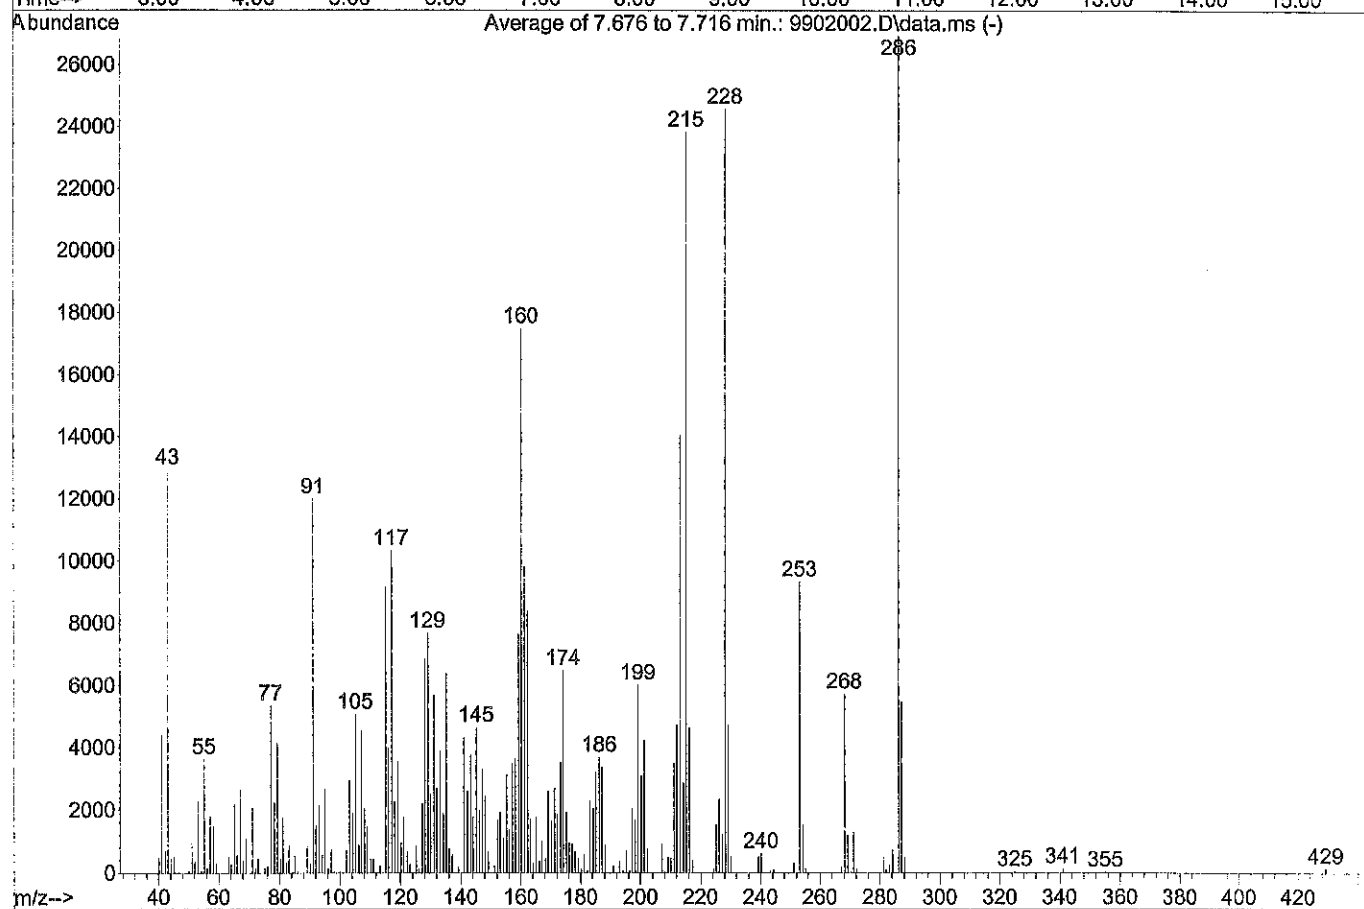


File : C:\MSDCHEM\1\DATA\2007\030628\9902002.D  
Operator : A.lisi  
Acquired : 28 Jun 2007 9:59 using AcqMethod FSSTER.M  
Instrument : nt03  
Sample Name: D916  
Misc Info :  
Vial Number: 99


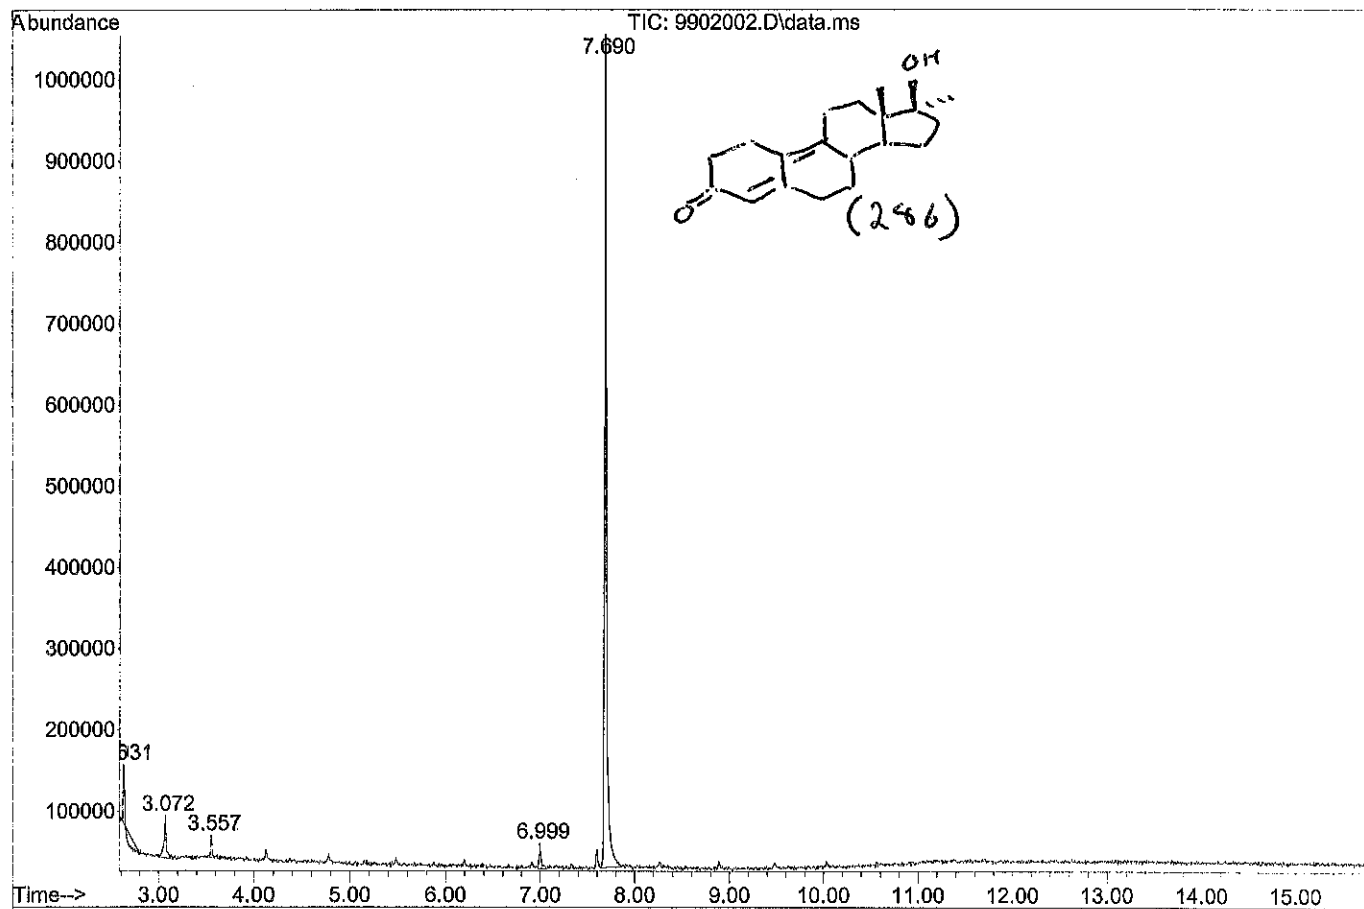


File : C:\MSDCHEM\1\DATA\2007\030628\9902002.D  
Operator : A.lisi  
Acquired : 28 Jun 2007 9:59 using AcqMethod FSSTER.M  
Instrument : nt03  
Sample Name: D916  
Misc Info :  
Vial Number: 99

17m HP2 80 (0.5 min)  
50°C to 200 (0.5 min)  
15°C to 310 (5 min)

inj 290

17m x 200µm x 0.25µm

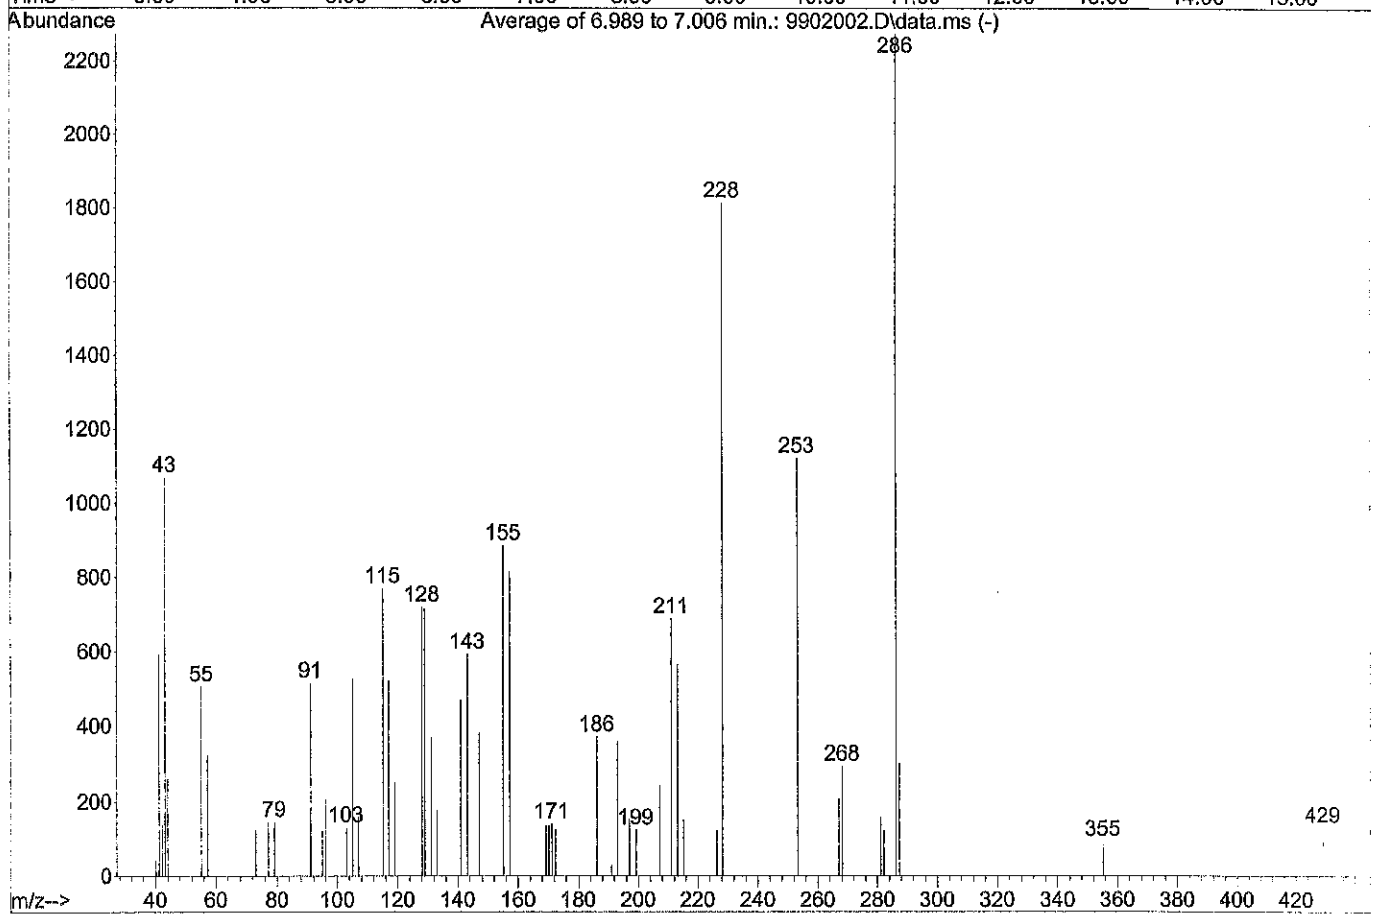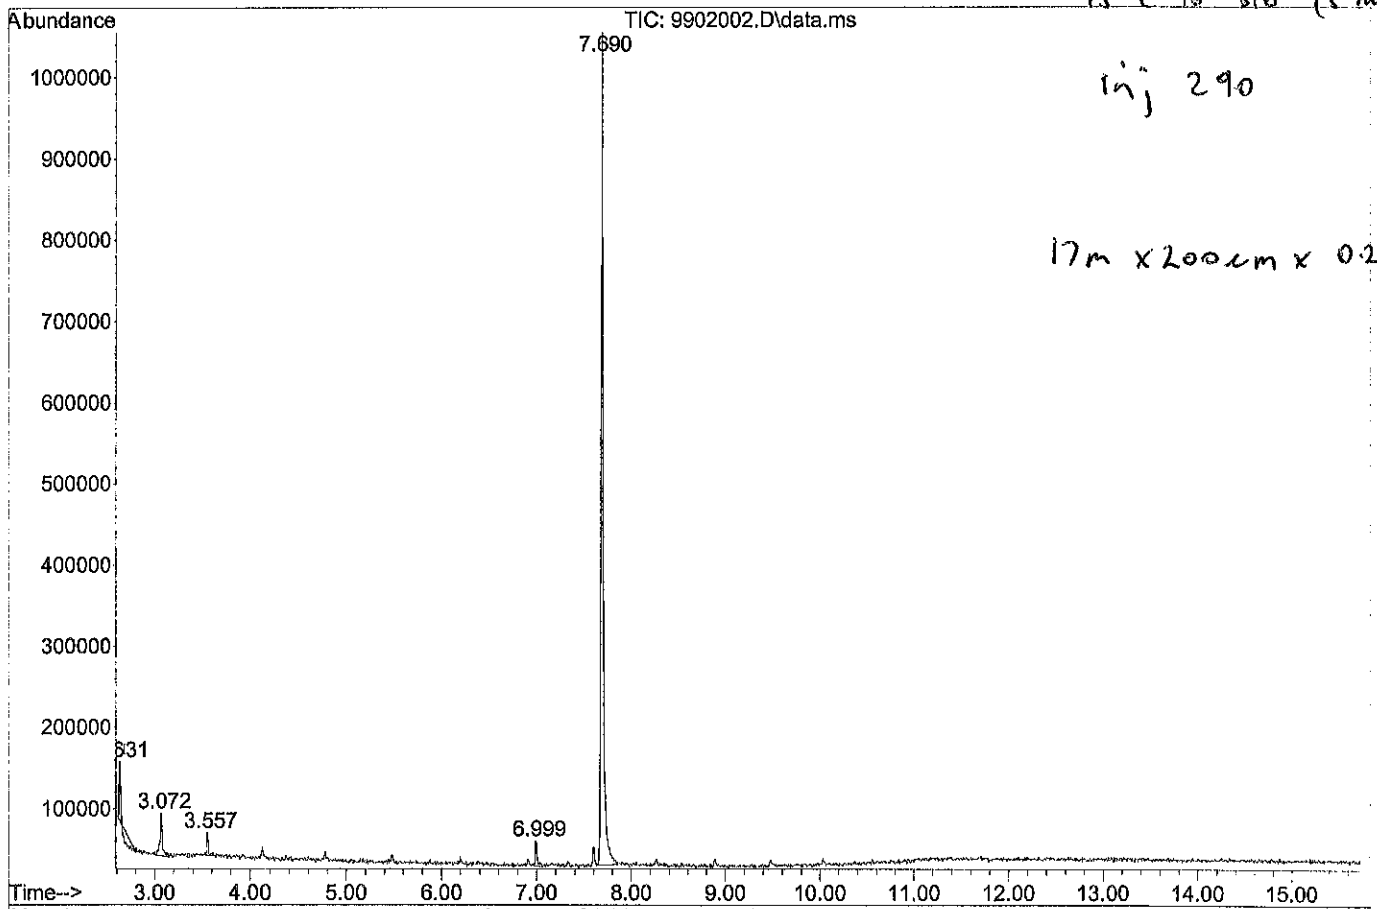

D916

Modified:subtracted

	m/z	Abundance
	41.15	16.0
	43.20	48.0
	53.20	9.0
	55.15	14.0
	57.15	7.0
	58.15	6.0
	65.15	8.0
	67.15	10.0
	71.20	8.0
	77.10	20.0
	78.15	8.0
X	79.15	15.0
	81.15	7.0
	91.15	45.0
	92.15	6.0
	93.15	8.0
	95.10	10.0
	103.10	11.0
	104.15	7.0
	105.15	19.0
	107.15	17.0
	108.15	8.0
	109.10	5.0
	115.10	34.0
	116.10	15.0
	117.15	38.0
	118.10	8.0
	119.15	13.0
	121.15	7.0
	127.15	8.0
	128.15	26.0
	129.10	29.0
	130.10	9.0
	131.10	21.0
	132.15	10.0
	133.05	14.0
	134.15	7.0
	135.15	24.0
	141.10	16.0
	142.20	10.0
	143.15	14.0
	144.10	7.0
	145.15	17.0
	146.15	7.0
	147.10	12.0
	148.10	9.0
	152.15	6.0
	153.15	7.0
	155.15	12.0
	156.15	5.0
	157.10	13.0
	158.10	14.0
	159.15	29.0
	160.15	65.0
	161.10	37.0
	162.15	31.0
	163.10	6.0
	165.15	7.0
	169.15	10.0
	170.15	6.0
	171.15	10.0
	172.15	7.0
	173.15	13.0
	174.15	24.0
	175.20	7.0
	183.15	9.0
	184.20	8.0
	185.15	12.0
	186.20	14.0
	187.15	13.0
	197.15	8.0
	198.15	6.0
	199.15	22.0
	200.20	11.0
	201.20	16.0
	211.15	13.0
	212.15	18.0
	213.20	52.0
	214.20	11.0
	215.20	88.0
	216.20	17.0
	225.15	6.0
	226.20	9.0
	227.20	5.0
	228.20	91.0
	229.20	18.0
	253.20	35.0
	254.20	6.0
	268.20	21.0
	271.25	5.0
	286.25	100.0
	287.25	21.0