
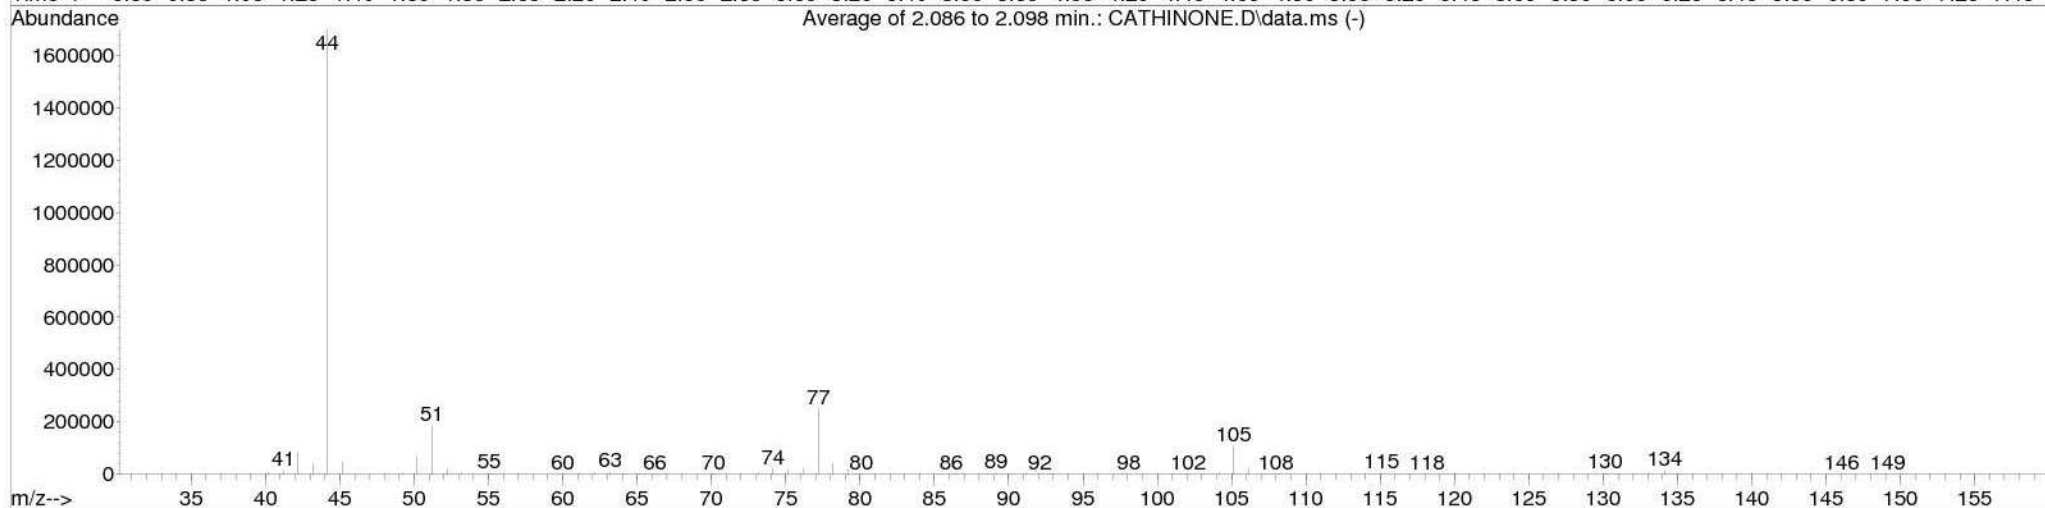


Name of File: D:\Data\JABPDF\00Edited\CATHINONE.D  
Method: 90\_1\_30.M  
Misc Info: DEA SWL

Vial Number: 94  
Instrument: DEA# 361782

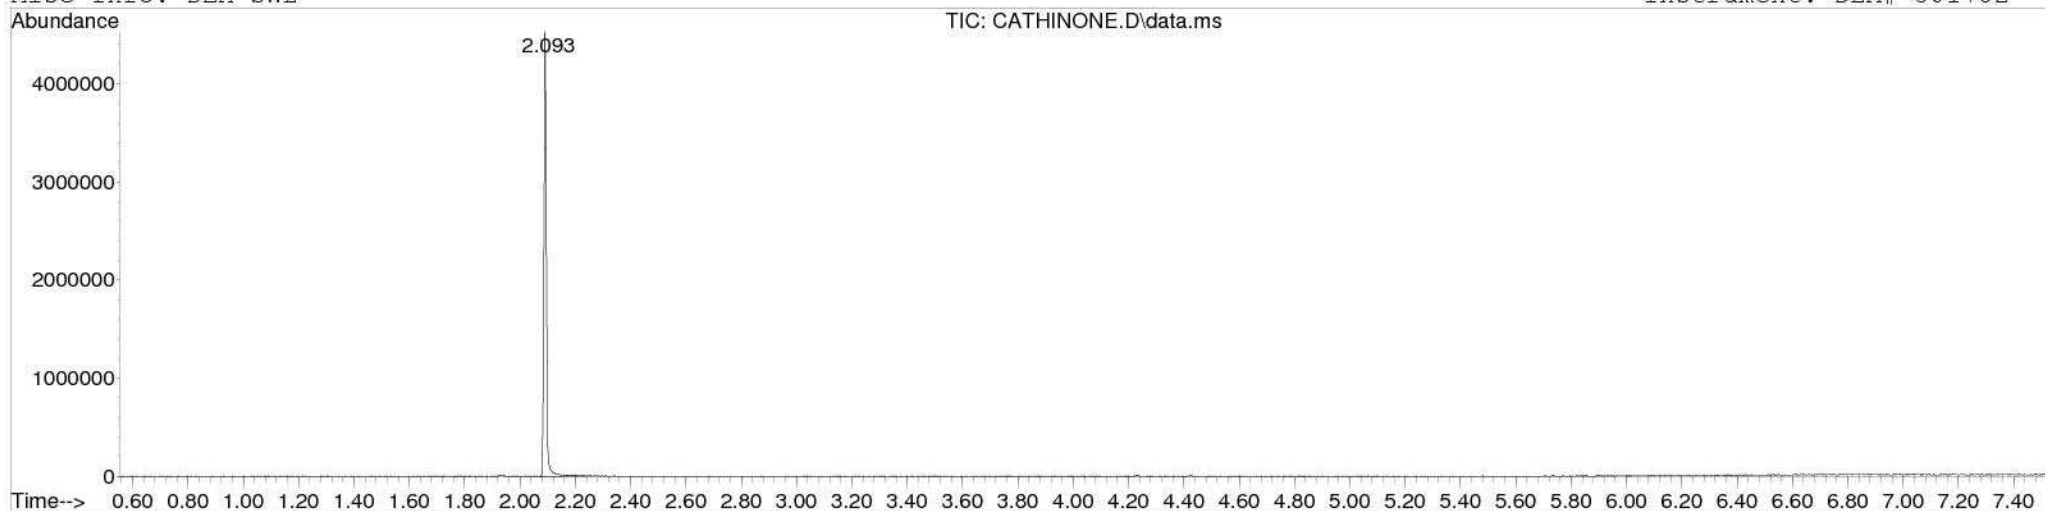

INSTRUMENT CONDITIONS

temp: 90 °C for 0.5 min  
then 38 °C/min to 300 °C for 1.7 min

Run Time 7.73 min

inj. port: 280 °C, transfer line: 280 °C

GC column: ZB-5MS: 15 m x 250 µm x 0.25 µm film

split mode: Split, ratio: 50 :1

tune: stune.u, multiplier offset: 0V

MS ACQUISITION PARAMETERS film

Laboratory Number: Cathnone STD

Date: 15 Sep 2005 11:44

Initials: \_\_\_\_\_